

implantswiss.com

NOVODENT SA
Y-Parc Technopole
Avenue des Sciences 11
CH-1400, Yverdon-les-Bains
Switzerland

05.2022 Rev.05

 **implantswiss**
SMART
CHOICE

IMPLANT TECHNOLOGY



» **IMPLANTSWISS
SHORT IMPLANTS**



SHORT IMPLANT

Short implants are considered as an alternative treatment to advanced surgical interventions in case of insufficient bone height, either above the mandibular canal or below the maxillary sinuses and aim to regenerate hard tissues.

Due to the aggressive thread design, Bone level short implants can preferably be used in the maxilla where the alveolar bone is relatively soft, whereas Tissue level short implants can be a good choice for the mandible.

BONE LEVEL

	$\varnothing 4.3$	$\varnothing 4.8$	$\varnothing 5.5$
Length	$\varnothing 4.3$	$\varnothing 4.8$	$\varnothing 5.5$
5.0 mm	S-BMFSR4305	S-BMFSR4805	S-BMFSR5505
6.0 mm	S-BMFSR4306	S-BMFSR4806	S-BMFSR5506


TISSUE LEVEL

	$\varnothing 4.3$	$\varnothing 4.8$	$\varnothing 5.5$
Length	$\varnothing 4.3$	$\varnothing 4.8$	$\varnothing 5.5$
4.0 mm	S-TFSR4304	S-TFSR4804	S-TWFSR5504
5.0 mm	S-TFSR4305	S-TFSR4805	S-TWFSR5505
6.0 mm	S-TFSR4306	S-TFSR4806	S-TWFSR5506

GH » 2.65 mm


SHORT IMPLANT SURGICAL KIT

The short surgical kit is recommended for both Bone and Tissue Level short implants.

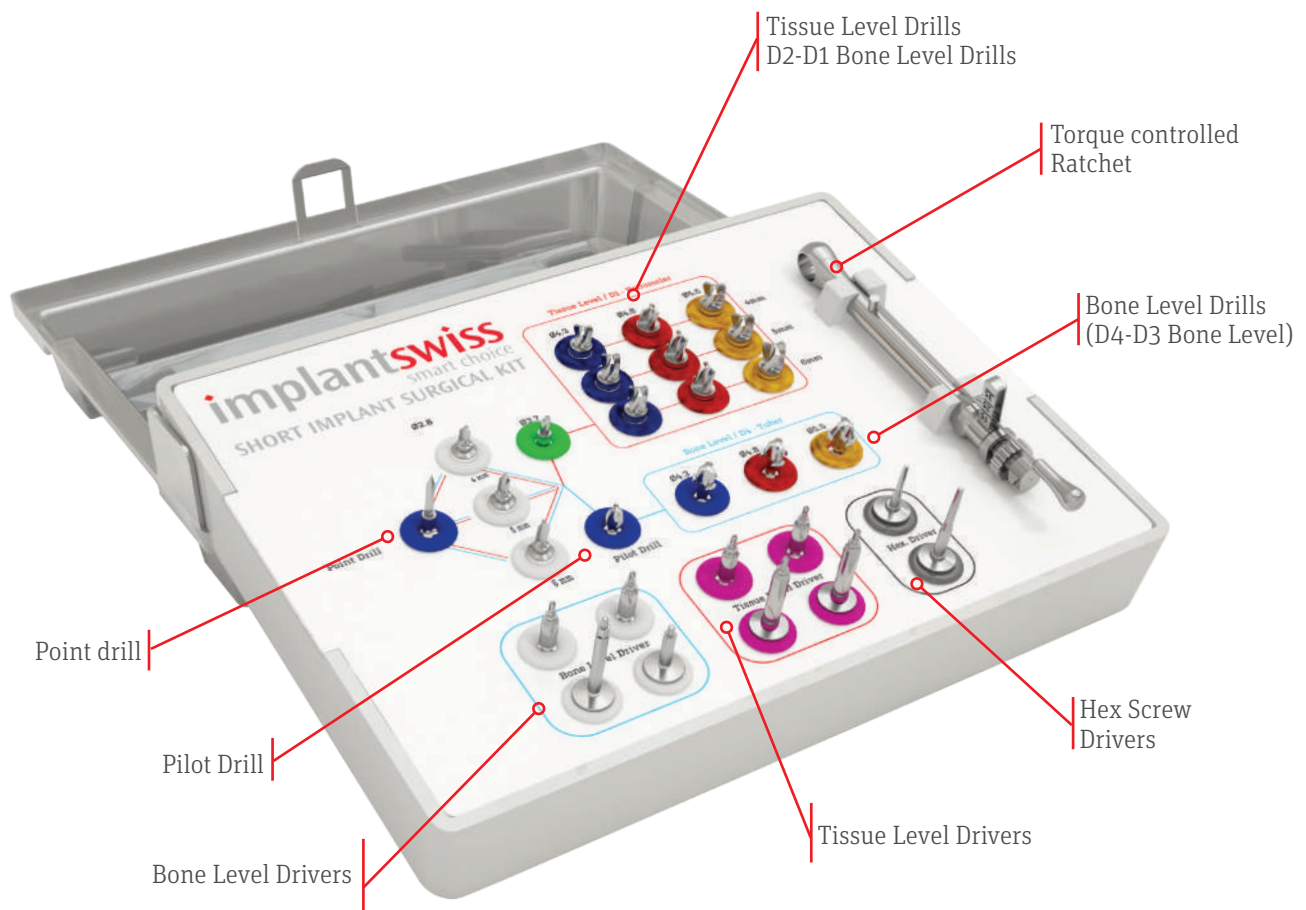


SHORT IMPLANT DRILLS & PROTOCOLS

The Implantswiss Short Implant Surgical Kit has a specific drill for each implant available in the system.

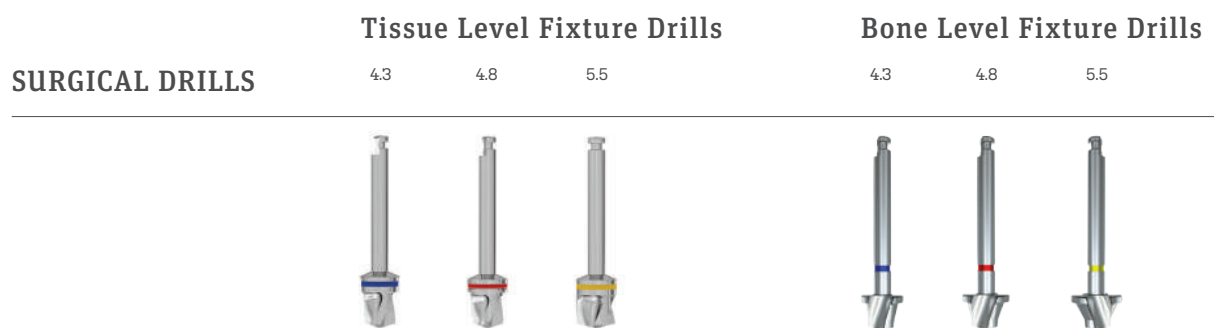

Implantswiss Short Implant Surgical Kit has various color-coded drills with different diameters and lengths. These drills are designed to simplify the surgical procedures resulting in shorter surgery time and less stress for the patients.

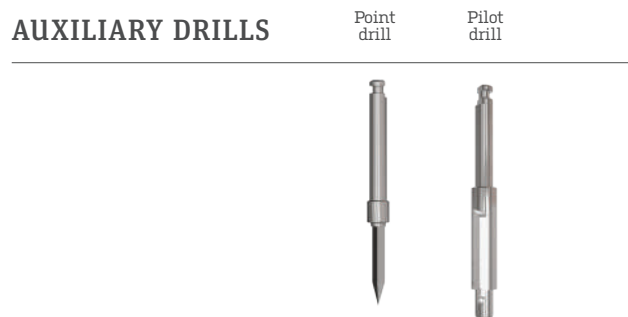


**ø4.3
Fixture**




BONE LEVEL

D4 / D3 Bone

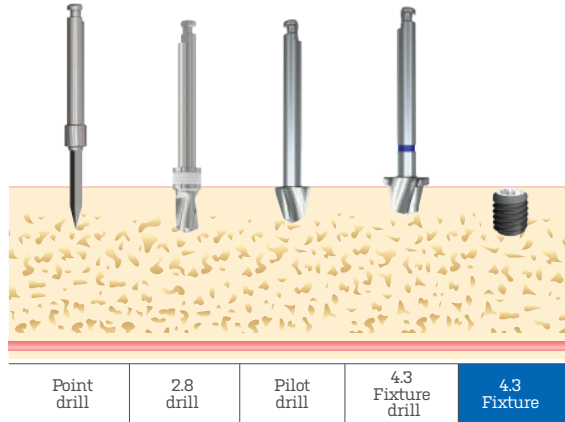


D2 / D1 Bone

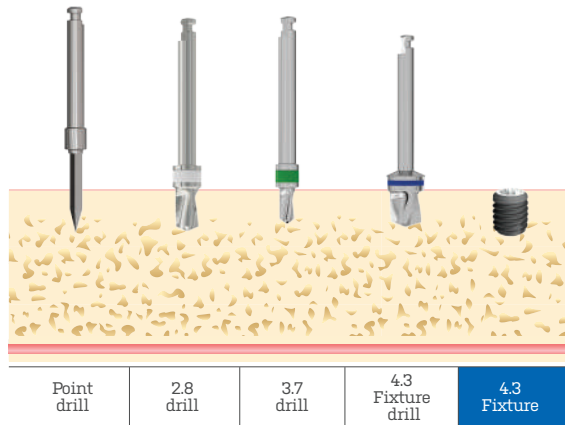

TISSUE LEVEL

D2 / D1 Bone

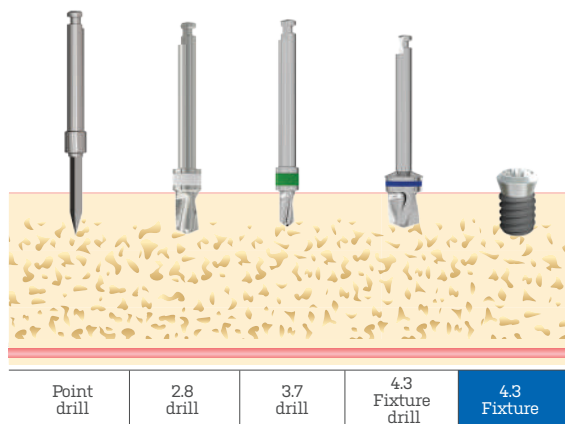


**ø4.8
Fixture**




BONE LEVEL

D4 / D3 Bone

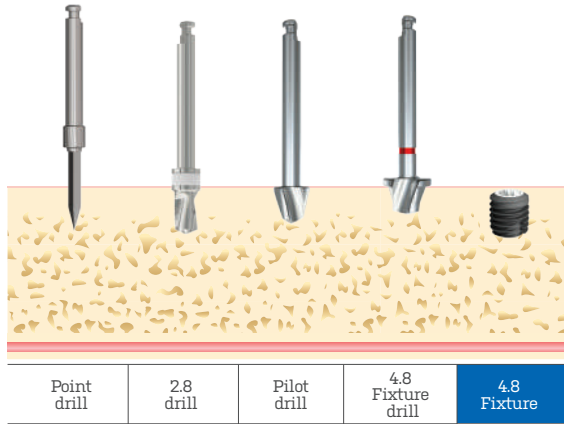


D2 / D1 Bone

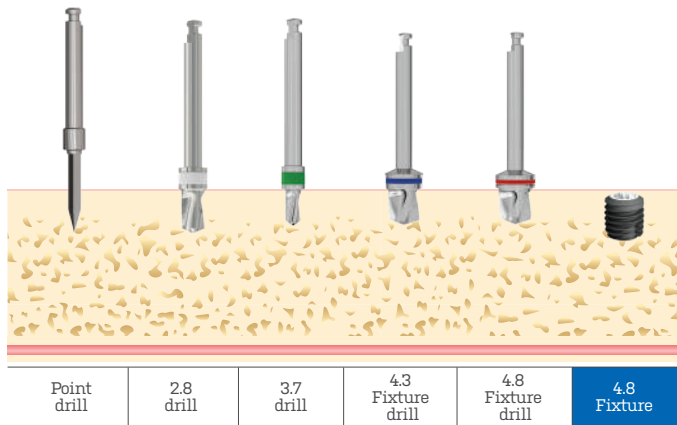

TISSUE LEVEL

D2 / D1 Bone

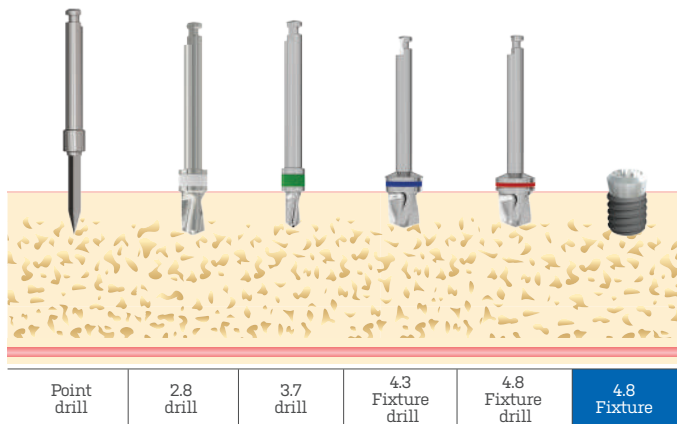


**ø5.5
Fixture**




BONE LEVEL

D4 / D3 Bone

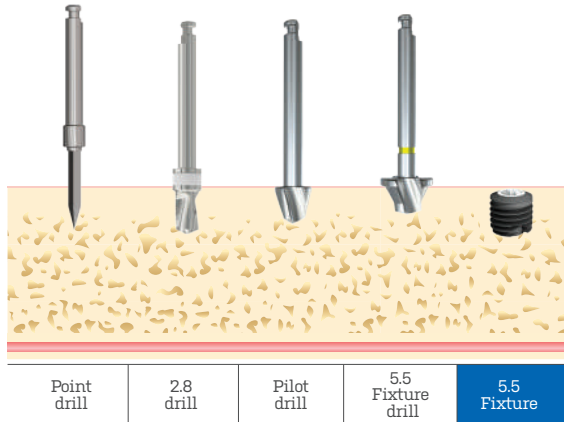


D2 / D1 Bone

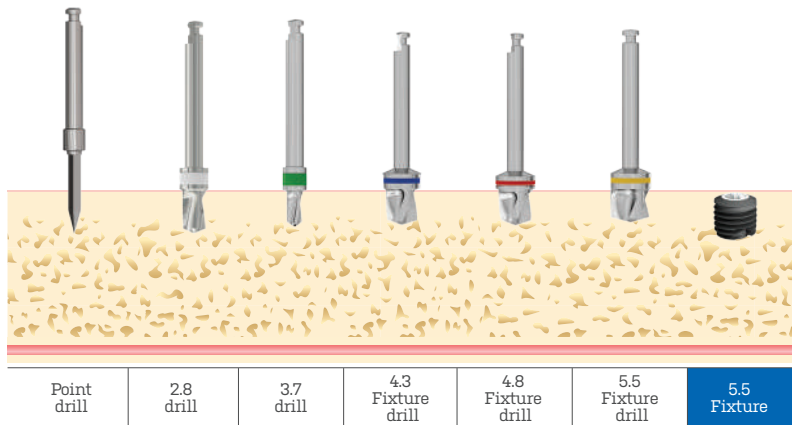

TISSUE LEVEL

D2 / D1 Bone

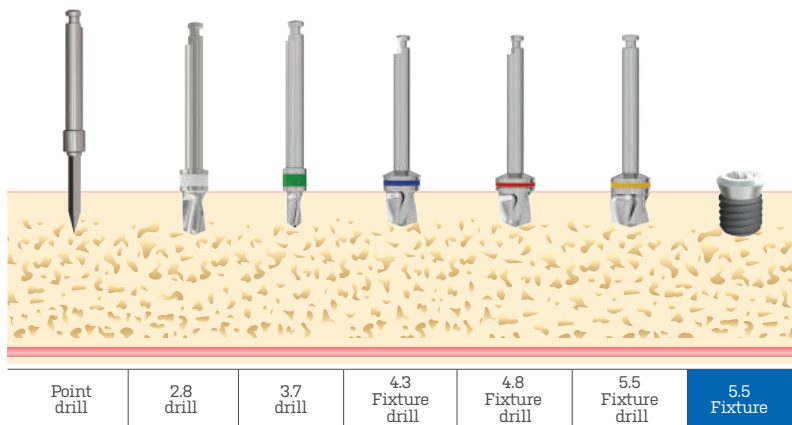




» **IMPLANTSWISS
PROSTHETIC COMPONENTS**



BONE LEVEL HEALING ABUTMENTS




BONE LEVEL SHORT IMPLANT HEALING ABUTMENTS

			
	Ø5.0	Ø6.0	Ø8.0
2 mm	S-BMHA5020	S-BMHA6020	S-BMHA8020
3 mm	S-BMHA5030	S-BMHA6030	S-BMHA8030

System » Bone Level
Material » Ti Grade 5 ELI
Driver » Hex Screw Driver



BONE LEVEL COUPLE SYSTEM

BONE LEVEL SHORT IMPLANT COUPLE ABUTMENTS

			
	Ø5.0	Ø6.0	Ø8.0
2 mm	S-BMCA5020	S-BMCA6020	S-BMCA8020
3 mm	S-BMCA5030	S-BMCA6030	S-BMCA8030

System » Bone Level
Material » Ti Grade 5 ELI
Torque Value » 25 Ncm
Driver » Hex Screw Driver

BONE LEVEL SHORT IMPLANT IMPRESSION COPING PICK UP

	
Ø5.0	Ø6.0
S-BMSICP50	S-BMSICP60

System » Bone Level
Material » Ti Grade 5 ELI

BONE LEVEL SHORT IMPLANT IMPRESSION COPING TRANSFER

	
S-BMSICT50	S-BMSICT60

System » Bone Level
Material » Ti Grade 5 ELI

BONE LEVEL FIXTURE LAB ANALOG


S-BMFLA

System » Bone Level
Material » Ti Grade 5 ELI



TISSUE LEVEL HEALING ABUTMENTS

TISSUE LEVEL HEALING ABUTMENTS



3.5 mm S-THA35
5.5 mm S-THA55



only for ø5.5 implant
S-THAW35
S-THAW55

System » Tissue Level
Material » Ti Grade 4
Torque Value » 20 Ncm
Driver » Hex Screw Driver

TISSUE LEVEL COUPLE SYSTEM

TISSUE LEVEL COUPLE ABUTMENTS



1 mm S-TCA10
2 mm S-TCA20
3 mm S-TCA30
4 mm S-TCA40



only for ø5.5 implant
S-TCAW10
S-TCAW20
S-TCAW30
S-TCAW40

System » Tissue Level
Material » Ti Grade 4
Torque Value » 25 Ncm
Driver » Hex Screw Driver

TISSUE LEVEL ANGLED ABUTMENT



15° S-TAA15
25° S-TAA25

System » Tissue Level
Material » Ti Grade 4
Torque Value » 25 Ncm
Driver » Hex Screw Driver

TISSUE LEVEL SYNOCTA ABUTMENT



6 mm S-TSOA

System » Tissue Level
Material » Ti Grade 4
Torque Value » 25 Ncm
Driver » Hex Screw Driver

TISSUE LEVEL IMPRESSION COPING PICK UP



OCTA S-TICP



only for ø5.5 implant
S-TICPW

System » Tissue Level
Material » Ti Grade 5 ELI

TISSUE LEVEL IMPRESSION COPING TRANSFER



OCTA S-TICT

System » Tissue Level
Material » Ti Grade 5 ELI

TISSUE LEVEL FIXTURE LAB ANALOG



S-TFLA



only for ø5.5 implant
S-TFLLA

System » Tissue Level
Material » Ti Grade 5 ELI



» **DIGITAL
SOLUTIONS**



BONE LEVEL

SCAN BODY



S-PMSB

System » Digital System
Driver » Hex Screw Driver

DIGITAL ANALOG



S-BMFDLA

System » Digital System
Driver » Hex Screw Driver

PREMILL



ø10 mm S-BMPA10
ø14 mm S-BMPA14
ø16 mm

System » Digital System
Material » Ti Grade 5 ELI
Driver » Hex Screw Driver

TISSUE LEVEL

SCAN BODY



S-TSB



only for ø5.5 implant
S-TWSB

System » Digital System
Driver » Hex Screw Driver

DIGITAL ANALOG



S-TFDLA



only for ø5.5 implant
S-TWFDLA

System » Digital System
Driver » Hex Screw Driver

PREMILL



ø10 mm S-TPA10
ø14 mm S-TPA14
ø16 mm S-TPA16



only for ø5.5 implant
S-TWPA10
S-TWPA14
S-TWPA16

System » Digital System
Material » Ti Grade 5 ELI
Driver » Hex Screw Driver



